


Redox XPS results for Bi 4f peaks. XPS narrowscan spectra (a) measured data in red and automatically-fitted data in blue, and (b) components of the automatic fit in red and orange, on fitted background in purple.

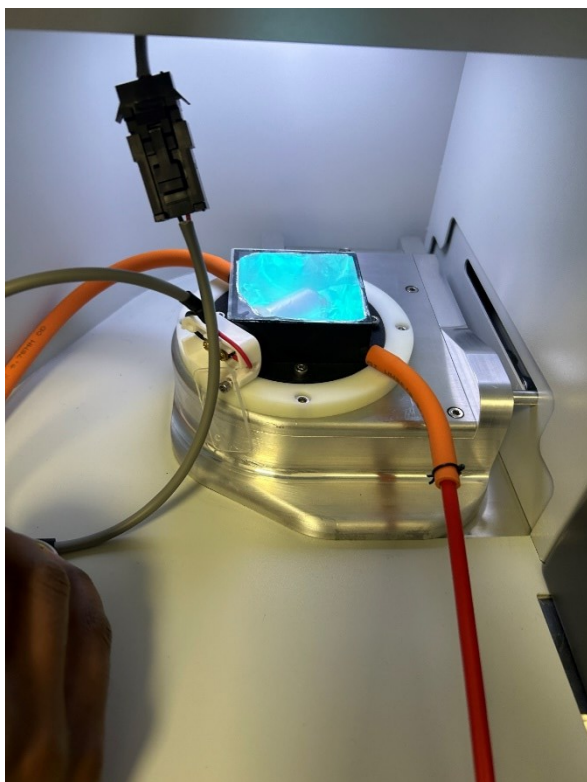

UV/ozone exposure proxime situ in the XPS instrument (ThermoFisher K-Alpha).